

# Momentum Health Technologies

17/34 Thynne  
St Bruce ACT  
2617 Australia

Hours of Operation  
Mon-Fri  
8:30am – 5:00pm (AEDT)

T: (02) 6210 0066  
E: orders@momentumht.com.au



## FEAFO Order Form

<b>Ship To:</b>	Customer Account No.:
	Purchase Order No.:
	Clinician:
Date Due:	Contact Telephone:
Urgent? <i>*Rush orders may attract an additional fee</i>	<b>Pt. Name/Reference:</b>

### Patient Details

Weight:                      Height:

### Orthosis Details

Left                      Right                      Bilateral

Foot Length:              cm

Encapsulated Plastic Thickness:

Encompass Malleoli with Plastic:

Encompass Met Head with Plastic:

### Sole Details

Heel Raise:                      Raise Height:              cm

Heel Post:

EVA Walking Sole:

### Additional Instructions

### Cosmetic Details

External Colour:

Strap Colour:

### Padding Details

*Foam Lining is intrinsic to a FEAFO, do you require additional Padding?*


Malleoli Padding:

Plantar Padding:

Additional Notes:

Lateral View

Medial View

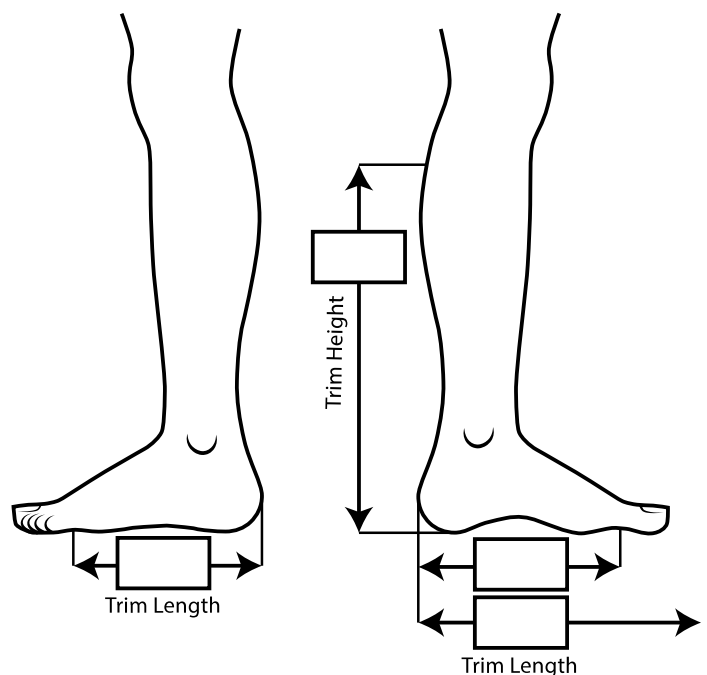

*Please note: No responsibility will be taken by Momentum Health Technologies for inappropriate or incorrect prescriptions. Devices will be made to the specifications identified on this form.*

# Momentum Health Technologies

6/28 Thynne St  
Bruce ACT  
2617 Australia

Hours of Operation  
Mon-Fri  
8:30am – 5:00pm (AEDT)

T: (02) 62100060  
F: (02) 61470239  
E: info@momentumht.com.au



## FEAFO Order Form

<b>Ship To:</b>	Customer Account No.:
	Purchase Order No.:
	Clinician:
<b>Date Due:</b>	Contact Telephone:
<b>Urgent?</b> <i>*Rush orders may attract an additional fee</i>	<b>Pt. Name/Reference:</b>

### Angular Cast Corrections

Goal Ankle Angle:            degrees or Neutral  
Goal Calcaneal Angle:        degrees or Neutral  
Goal Toe Spring:            degrees mm  
Shoe Pitch:            mm


### Specific Offloading

### Forefoot Corrections:


Abduction            or Adduction            to            degrees  
or neutral            as cast/scanned  
Rotation:            degrees or Neutral  
As cast/scanned

### Additional Instructions

### Anterior View

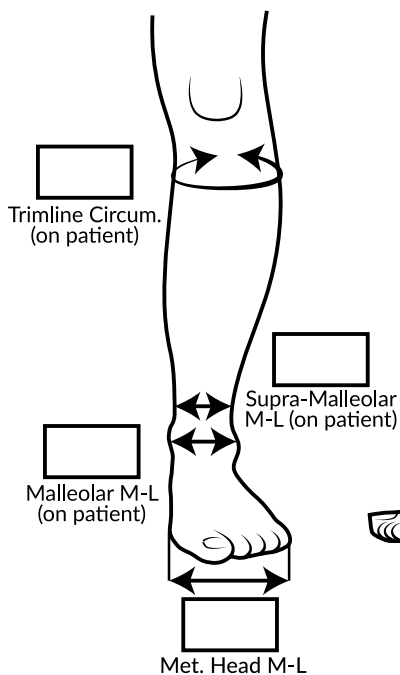

### Lateral/Medial Views

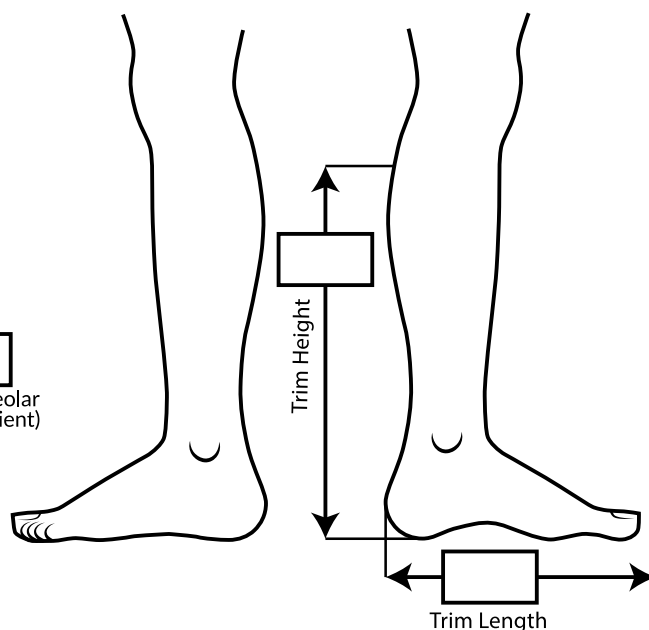

*Please note: No responsibility will be taken by Momentum Health Technologies for inappropriate or incorrect prescriptions. Devices will be made to the specifications identified on this form.*