

Momentum Health Technologies

17/34 Thynne St
Bruce ACT 2617
Australia

Hours of Operation
Mon-Fri
8:30am – 5:00pm (AEDT)

T: (02) 6210 0066
E: orders@momentumht.com.au



KAFO Order Form

Ship To:	Customer Account No.:
	Purchase Order No.:
	Clinician:
Date Due:	Contact Telephone:
Urgent? <i>*Rush orders may attract an additional fee</i>	Pt. Name/Reference:

Patient Details

Weight: Height:
Left Right Bilateral

PETG Check-Fit Device Required

Orthosis Details

Material Type:
Knee Joint: Ankle Joint:
Cable Unlock:
Forefoot:

Components

Please contact us for a complete range of Streifeneder components!

Knee Joint: (Including company & item code)

Ankle Joint: (Including company & item code)

Other Components stirrups/uprights etc (company & item code)

Trimline Details

Thigh:
Calf:
Foot Section: Contain Met Heads:

Strapping Details

Thigh:
Calf/Shin: Ankle:
Knee Spider:

Cosmetic Details

Thermoplastic

Paper Transfer:

Laminated

Carbon-Fibre Finish
Colour Pigment (additional lamination):
Fabric Covering (additional lamination):

Please Supply Fabric or Contact us for Options

Strap Colour:

Padding Details

Malleoli Padding:
Lining Material:
Plantar Padding:
Additional Padding:

Sole Details

Heel Raise: Raise Height: cm
Heel Post: EVA Walking Sole:

Additional Instructions

Please attached anterior and medial photos of KAFO to order

Please note: No responsibility will be taken by Momentum Health Technologies for inappropriate or incorrect prescriptions. Devices will be made to the specifications identified on this form.

Momentum Health Technologies

17/34 Thynne St
Bruce ACT 2617
Australia

Hours of Operation
Mon-Fri
8:30am – 5:00pm (AEDT)

T: (02) 6210 0066
E: info@momentumht.com.au



KAFO Order Form

Ship To:	Customer Account No.:
	Purchase Order No.:
	Clinician:
Date Due:	Contact Telephone:
Urgent? <i>*Rush orders may attract an additional fee</i>	Pt. Name/Reference:

Angular Cast Corrections

Goal Ankle Angle: deg
or Neutral As Cast/Scanned

Goal Calcaneal Angle: deg
or Neutral As Cast/Scanned

Goal Knee Flexion Angle: deg
or Neutral As Cast/Scanned

Goal Toe Spring: deg Shoe Pitch: mm

Toe-out Angle: deg
or Neutral As Cast/Scanned


Specific Offloading:

Additional Notes:

Forefoot Corrections

ABduction or ADDuction to deg
or Neutral as Cast/Scanned

Rotation to degrees
or Neutral as Cast/Scanned

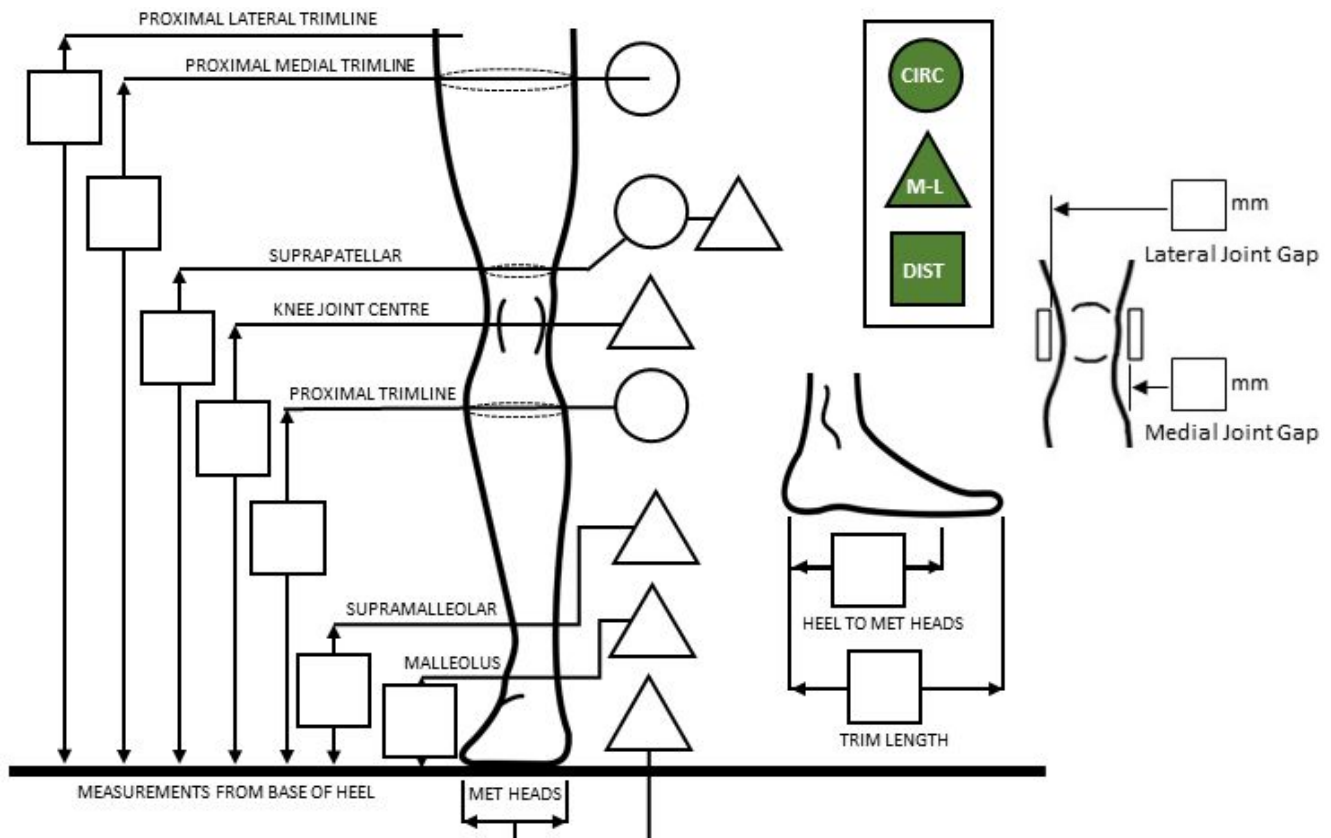

Please note: No responsibility will be taken by Momentum Health Technologies for inappropriate, incorrect or conflicting prescriptions. This may cause a delay in manufacturing until the information is clarified. Devices will be made to the specifications identified on this form.